

Portable Data/Video Processing Unit

FIG. 1A

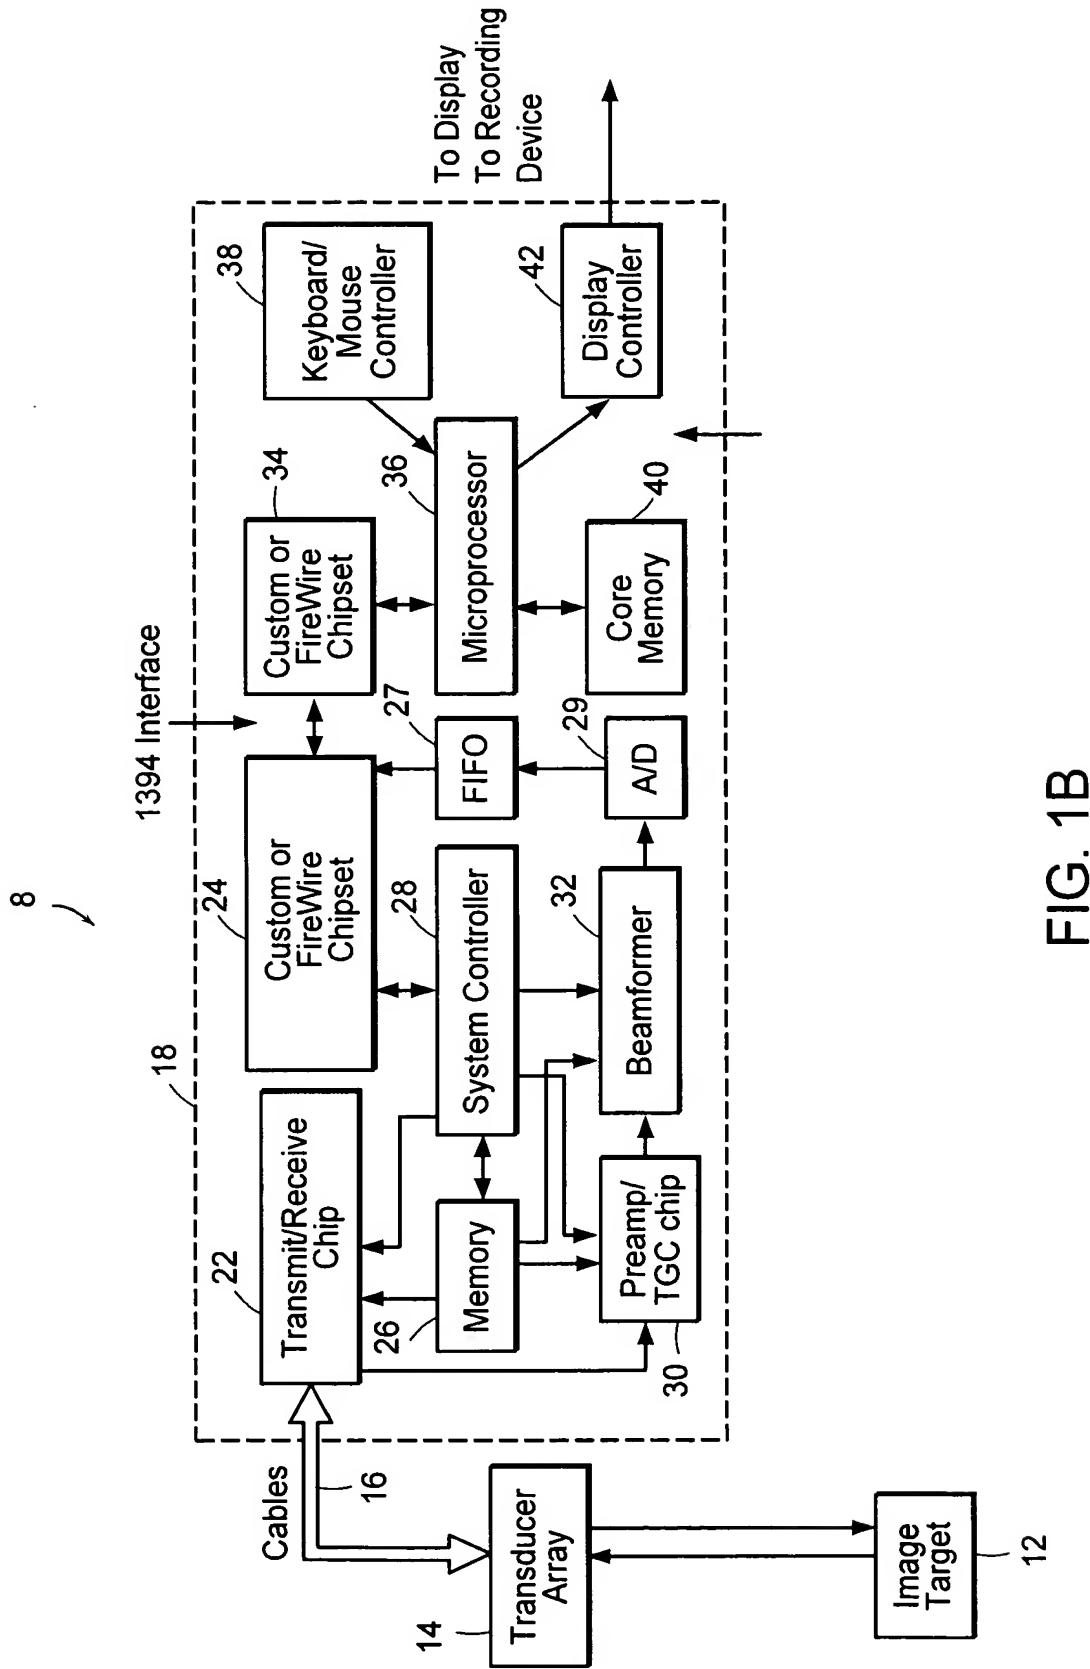


FIG. 1B


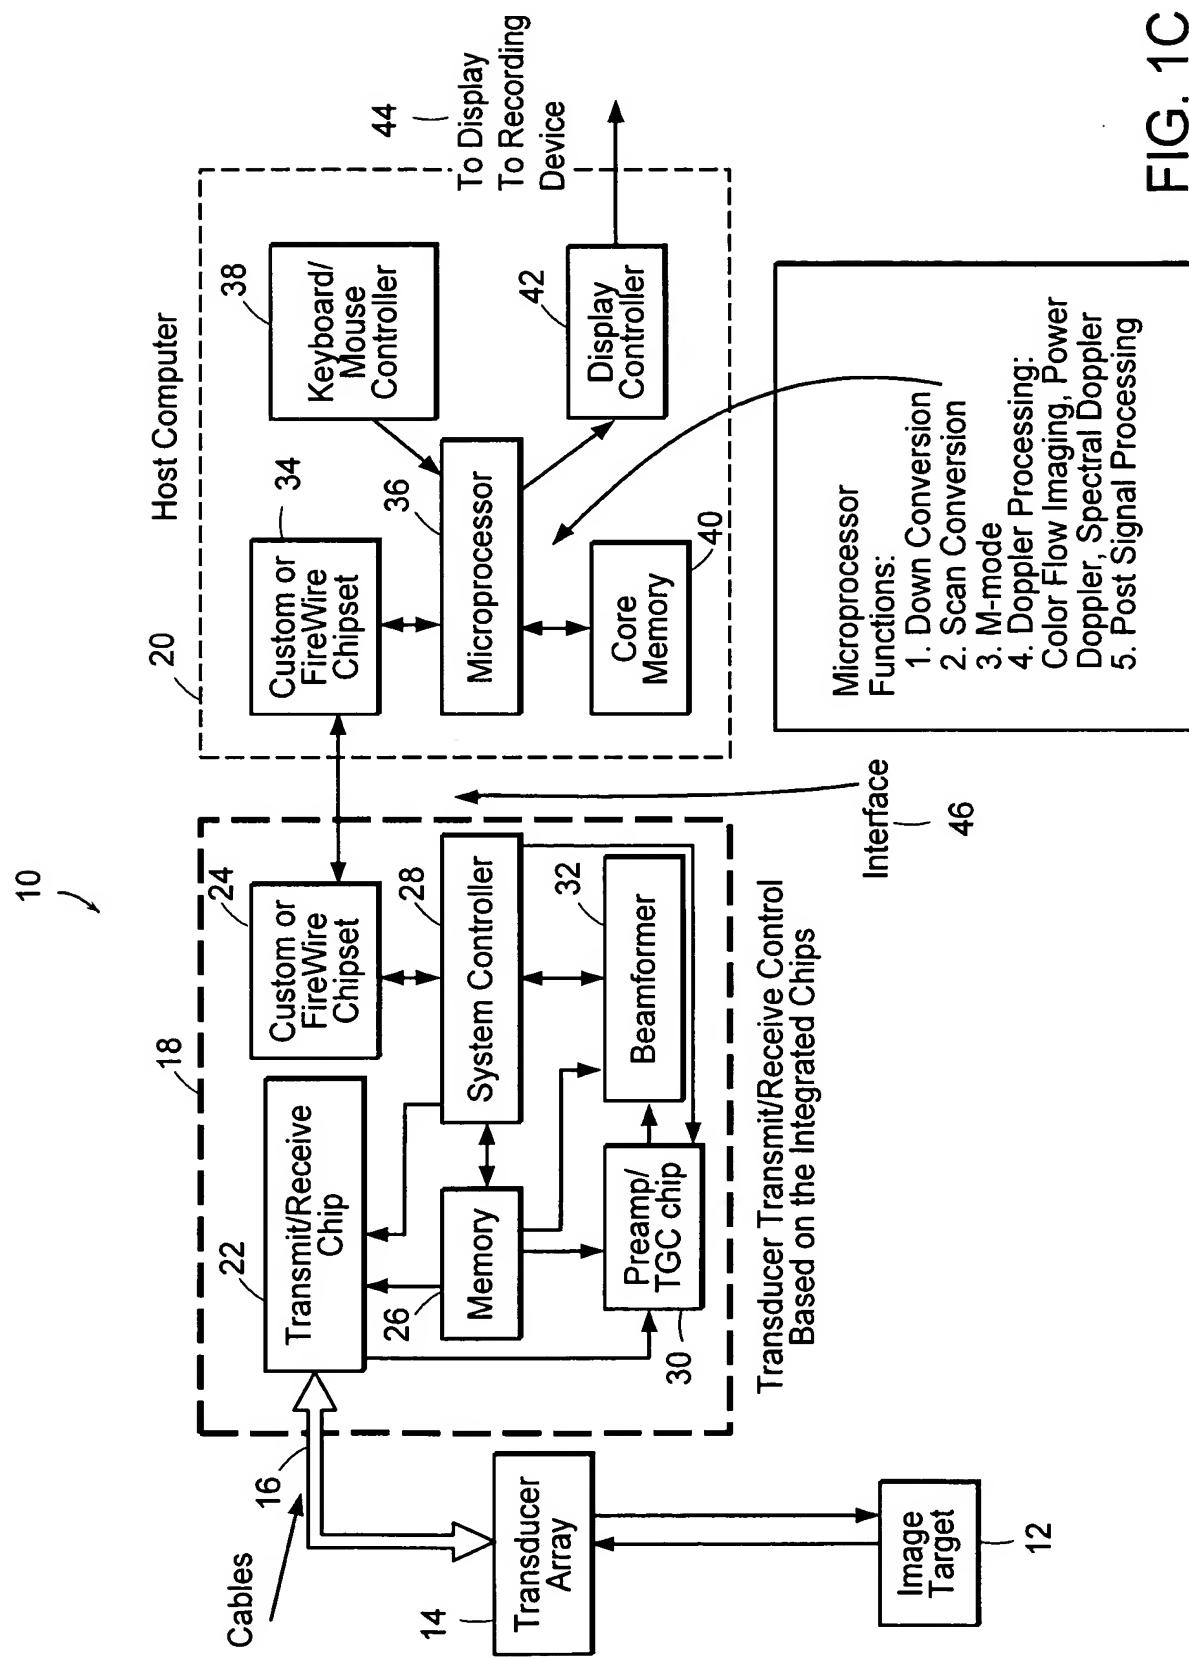


FIG. 1C

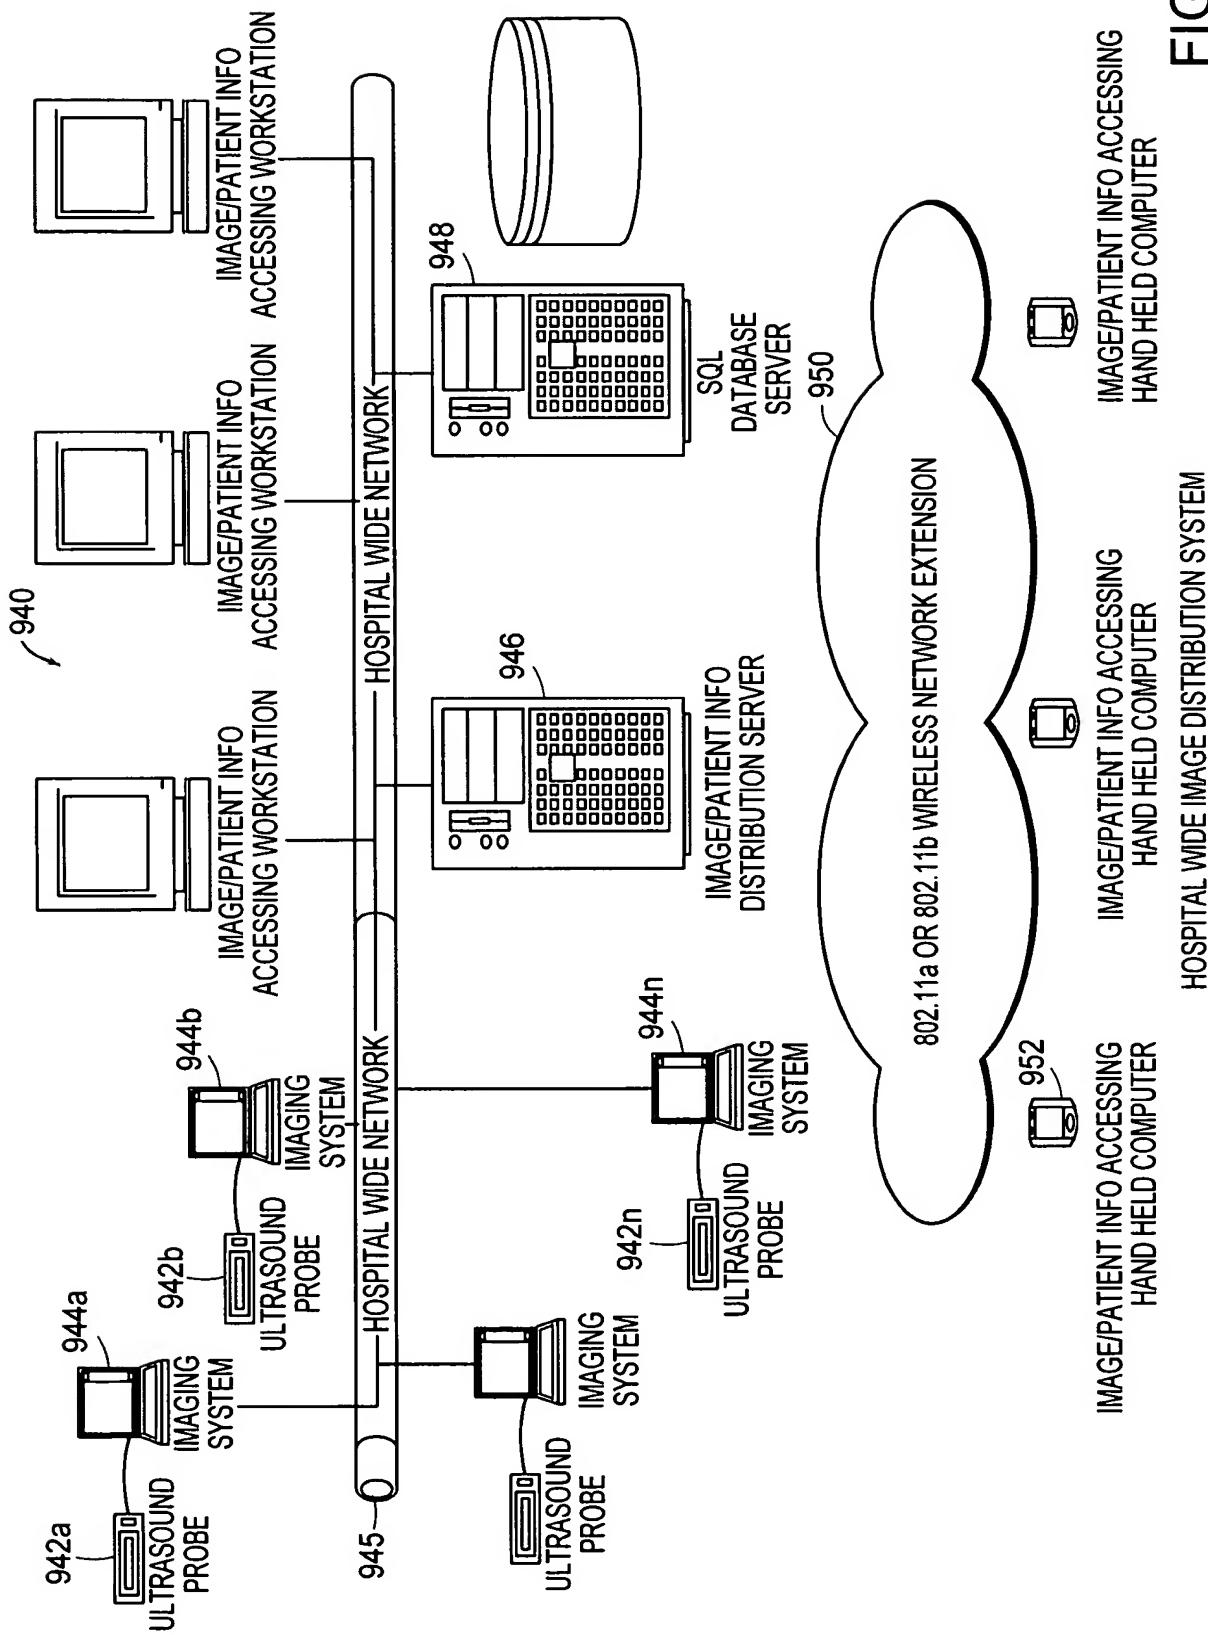

5/23

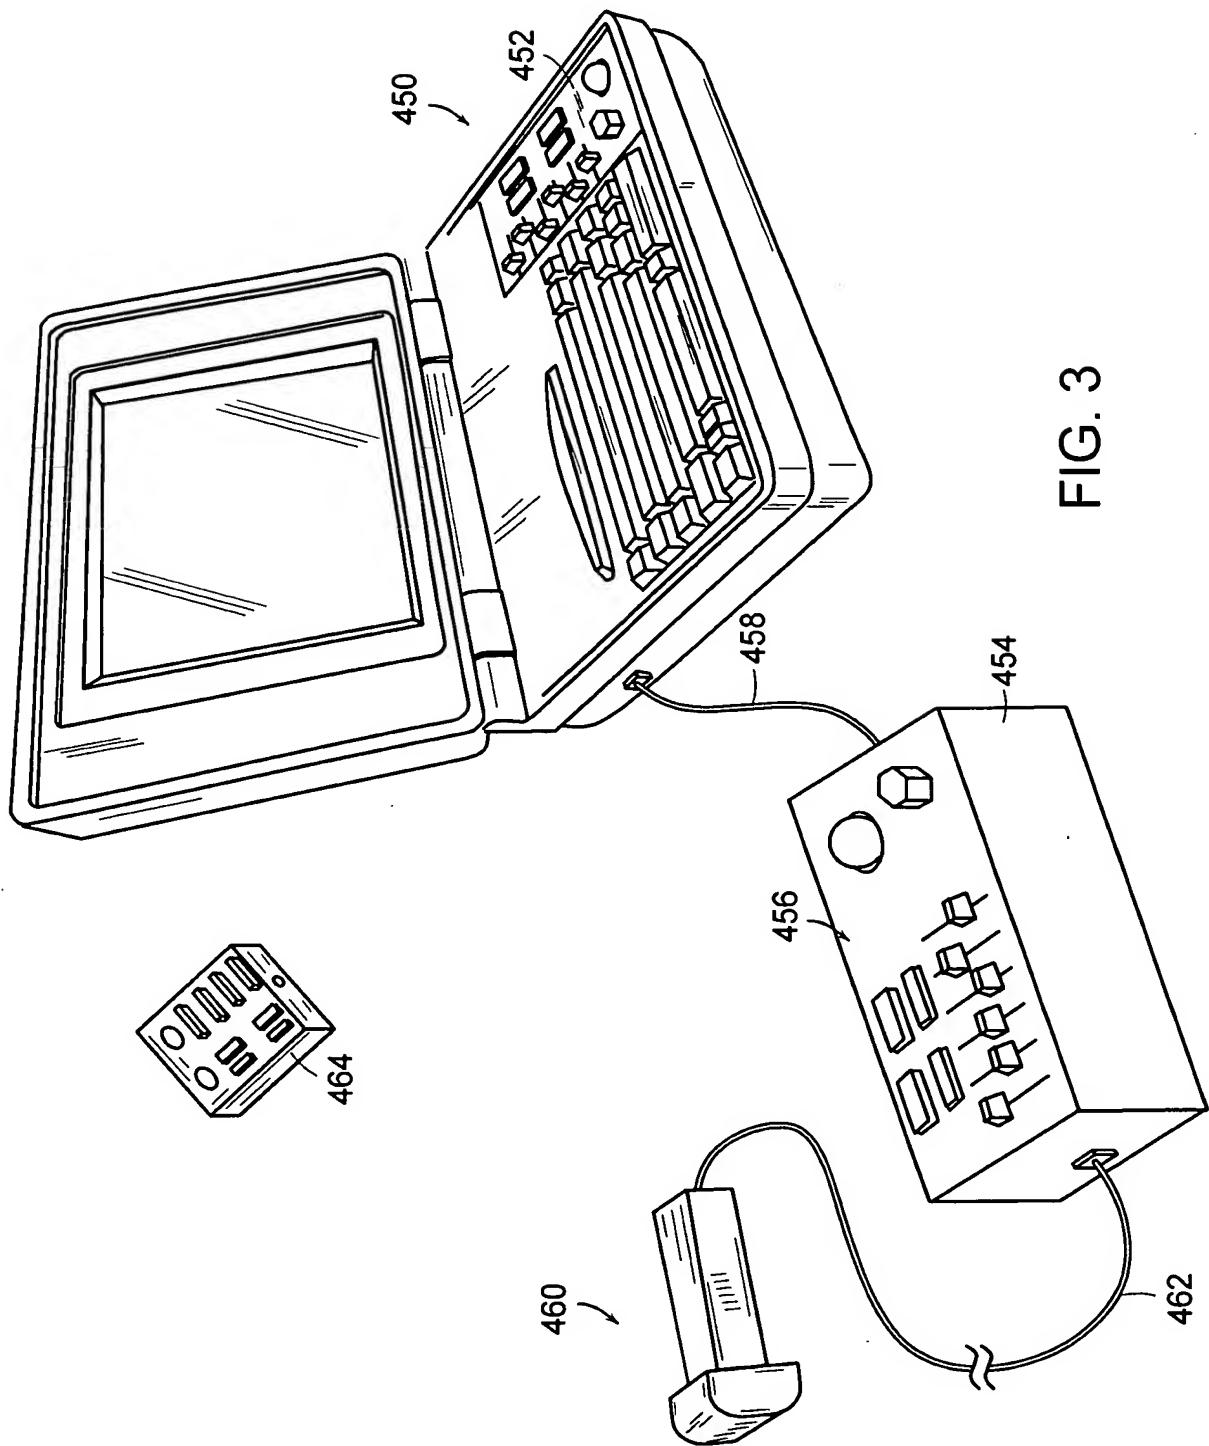


FIG. 3

6/23

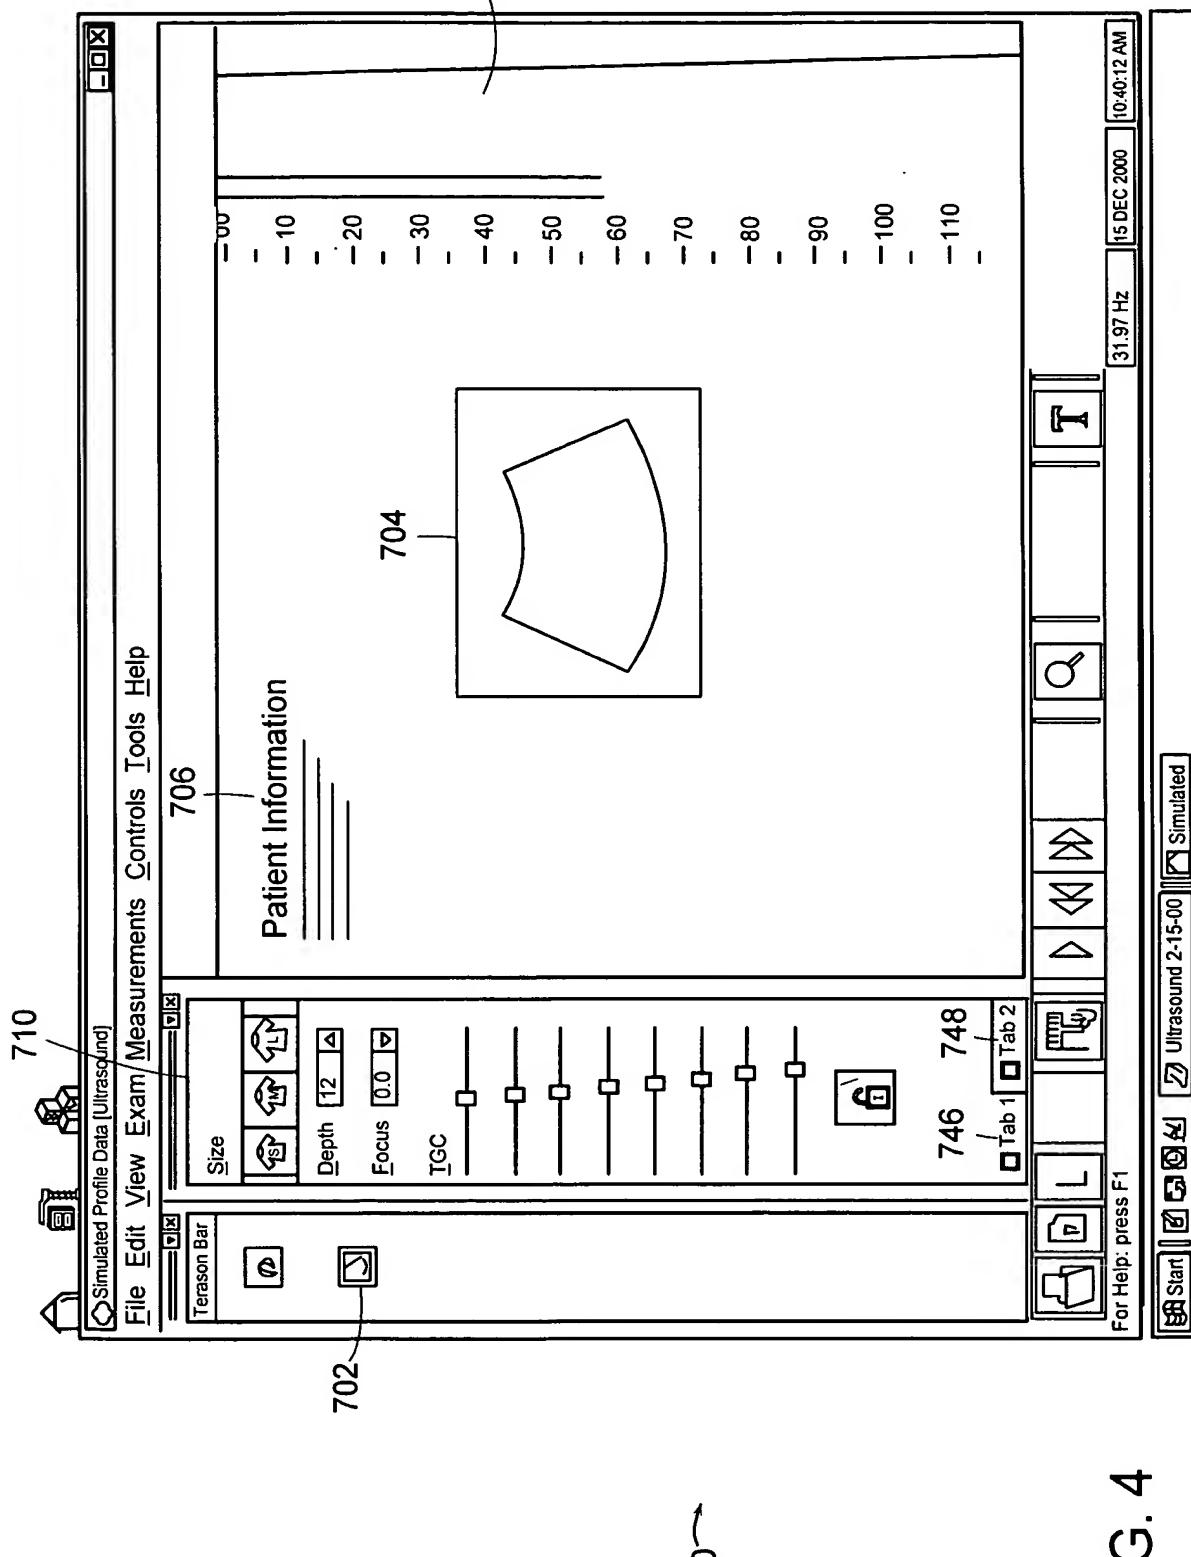


FIG. 4

7/23

Apical Four-Chamber Duplex or Triplex Tissue Doppler Imaging

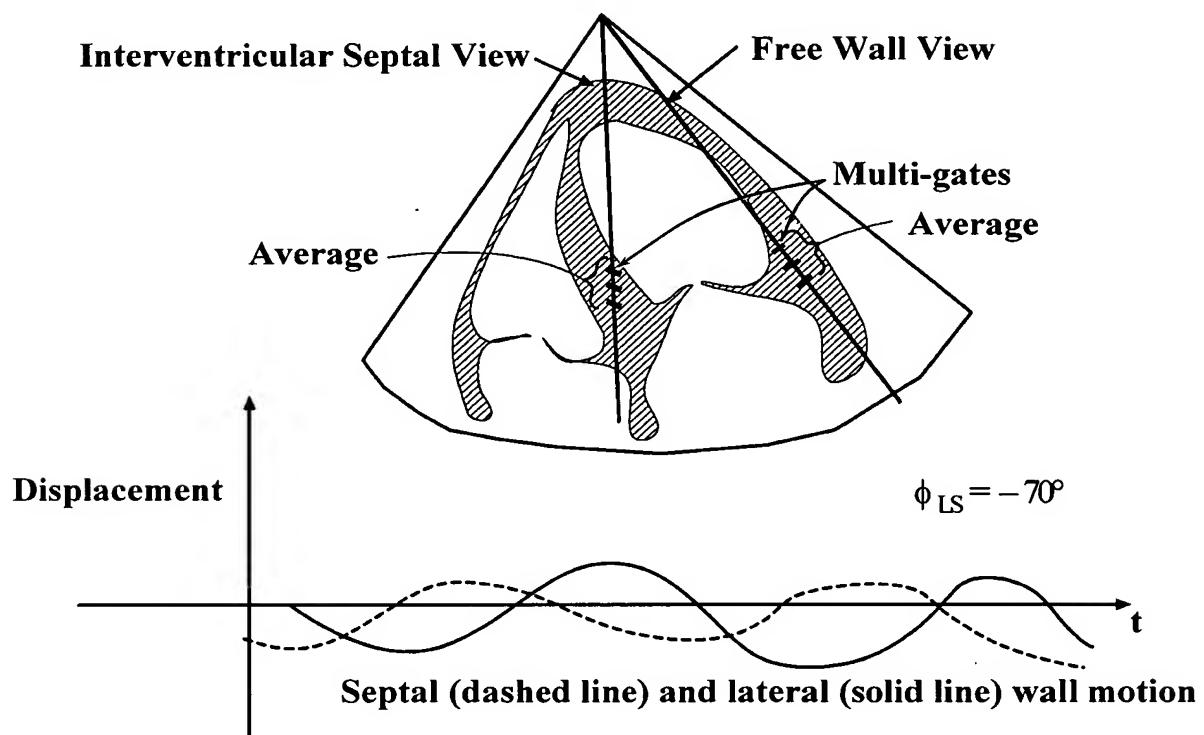


FIG. 5

8/23

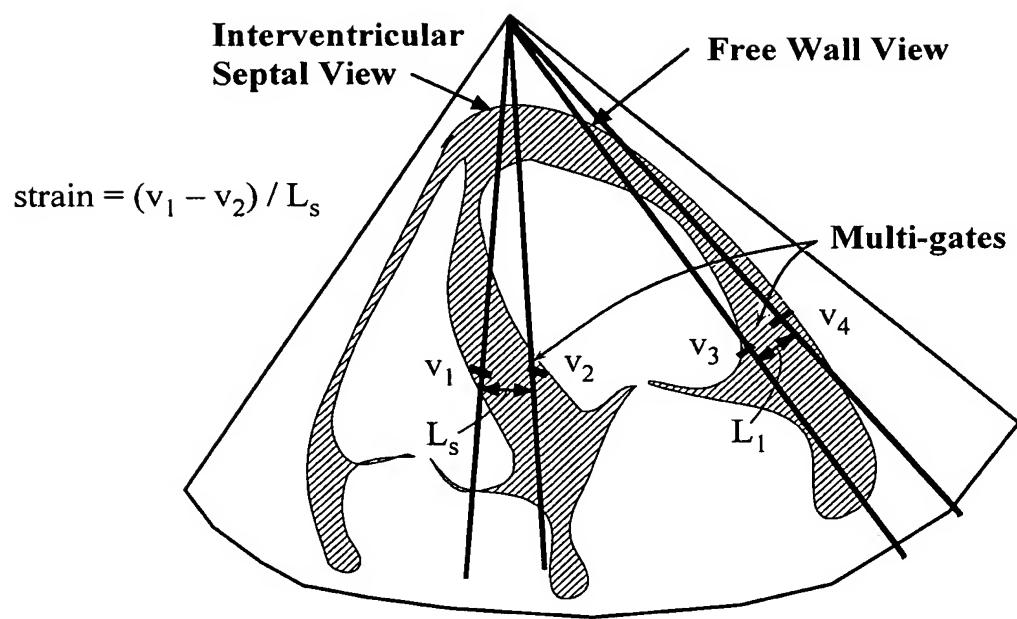


FIG. 6

9/23

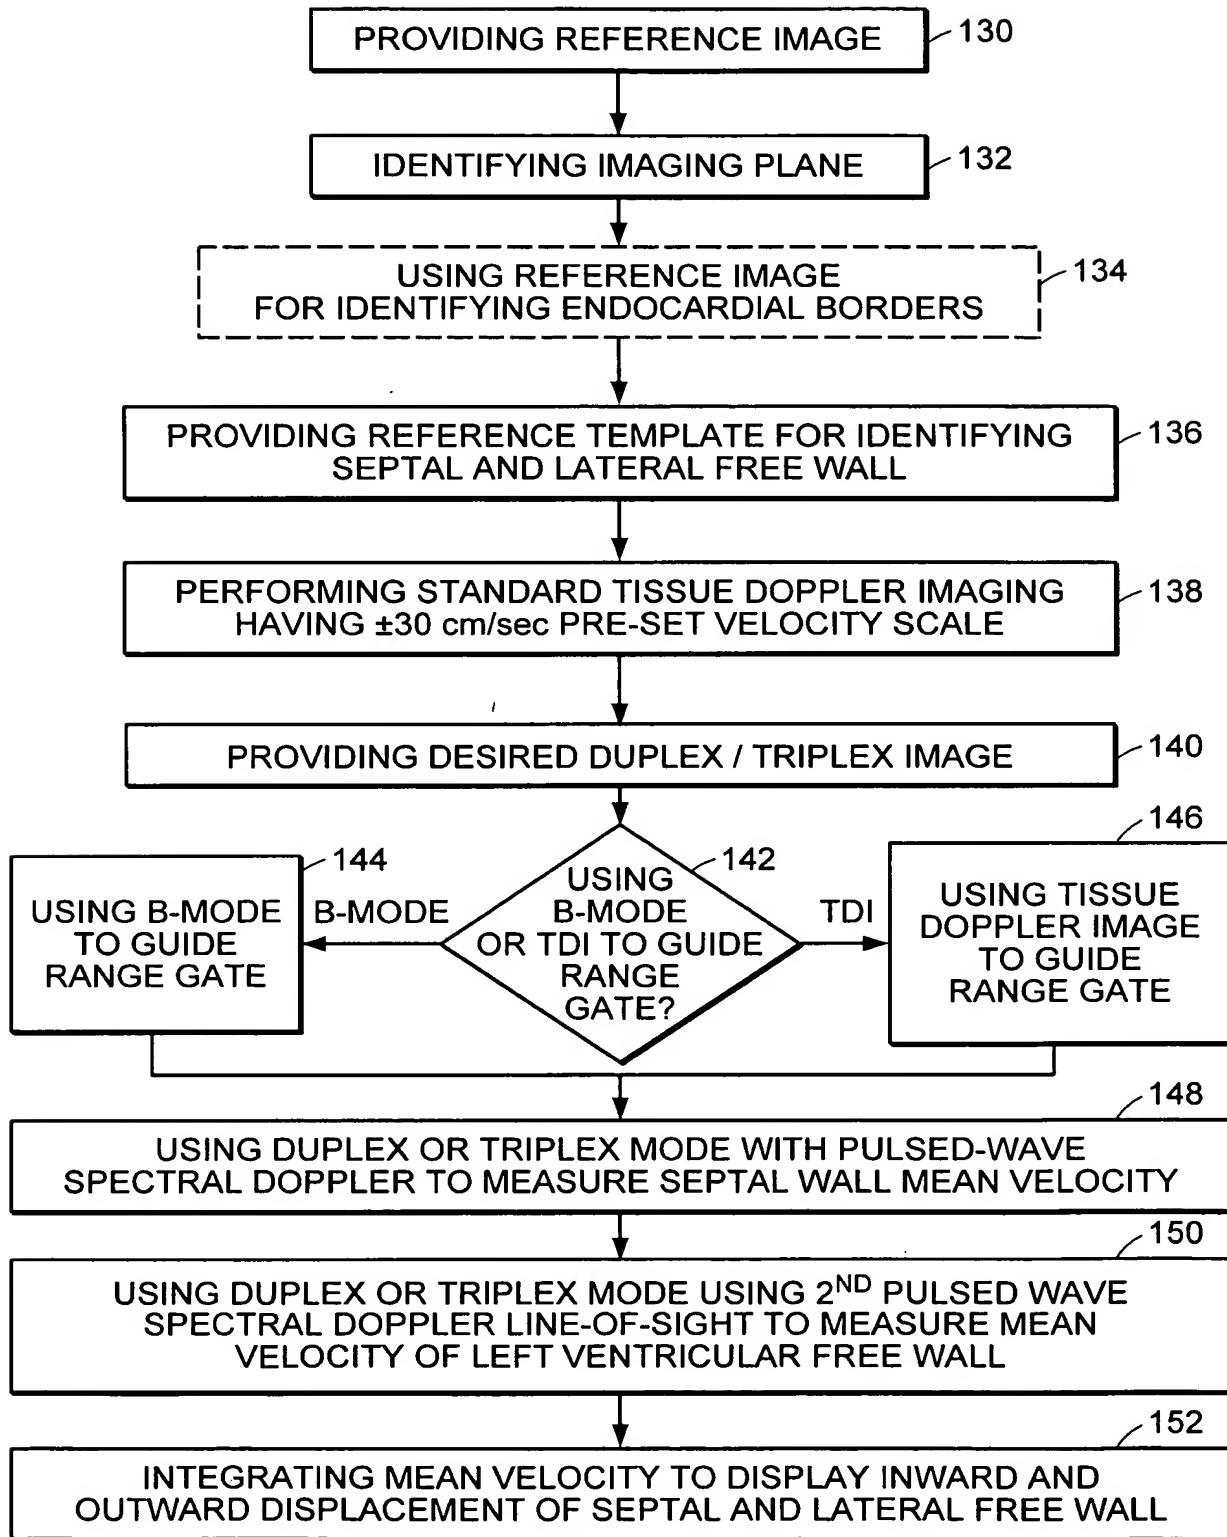


FIG. 7

10/23

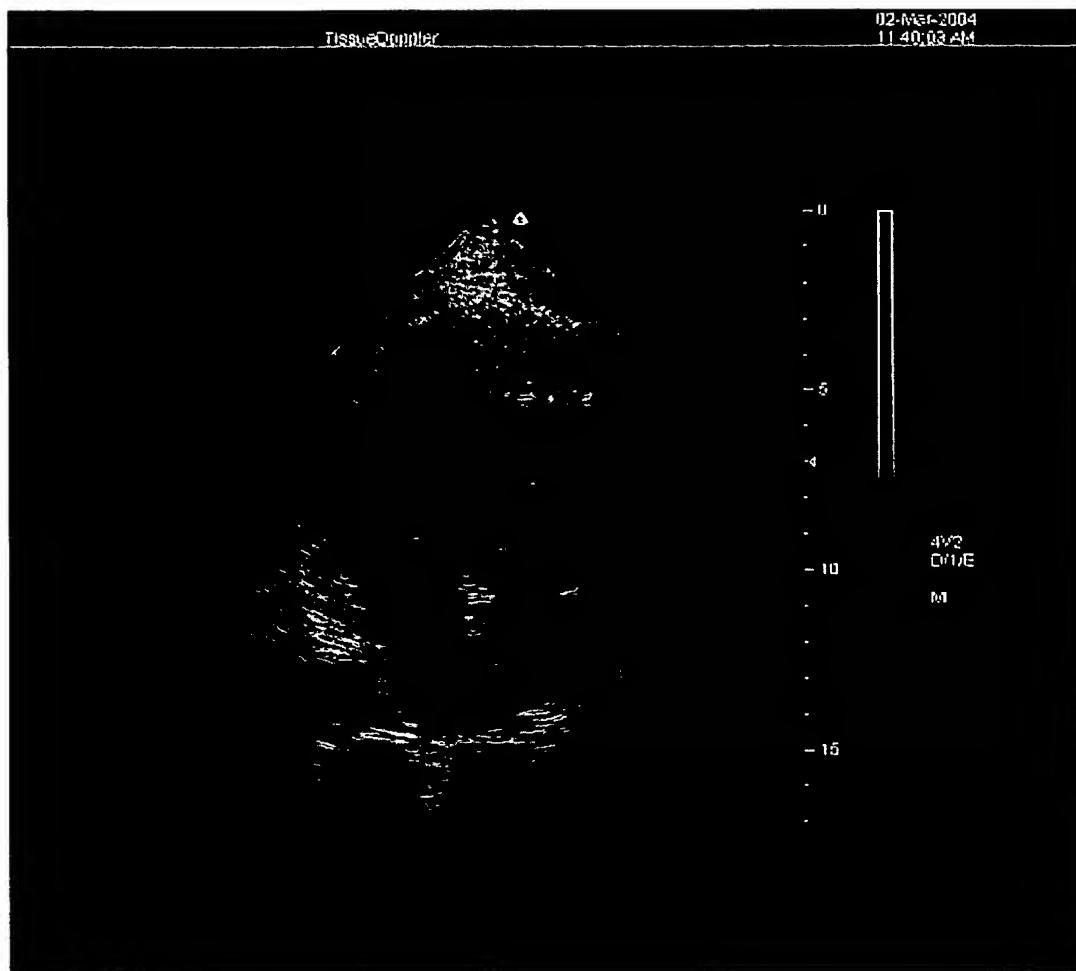


FIG. 8

11/23

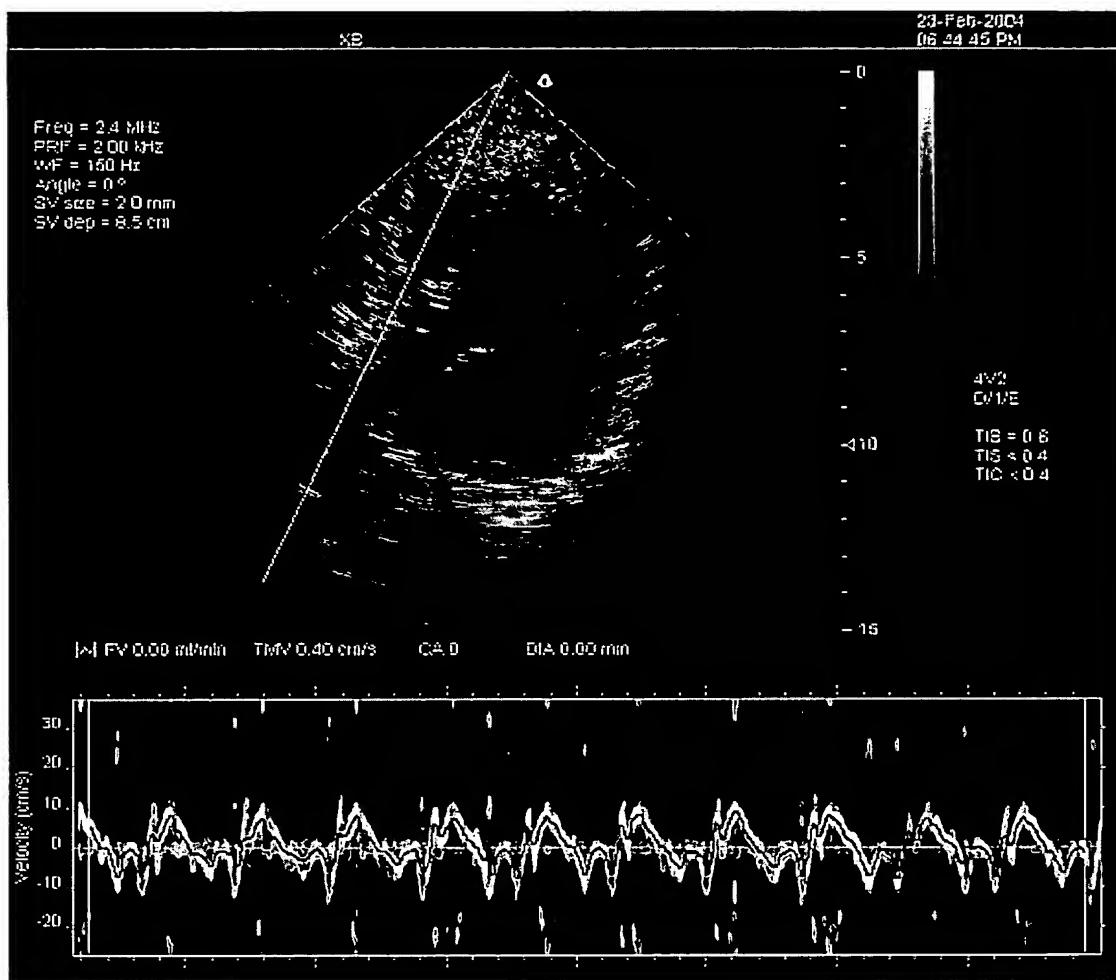


FIG. 9

12/23

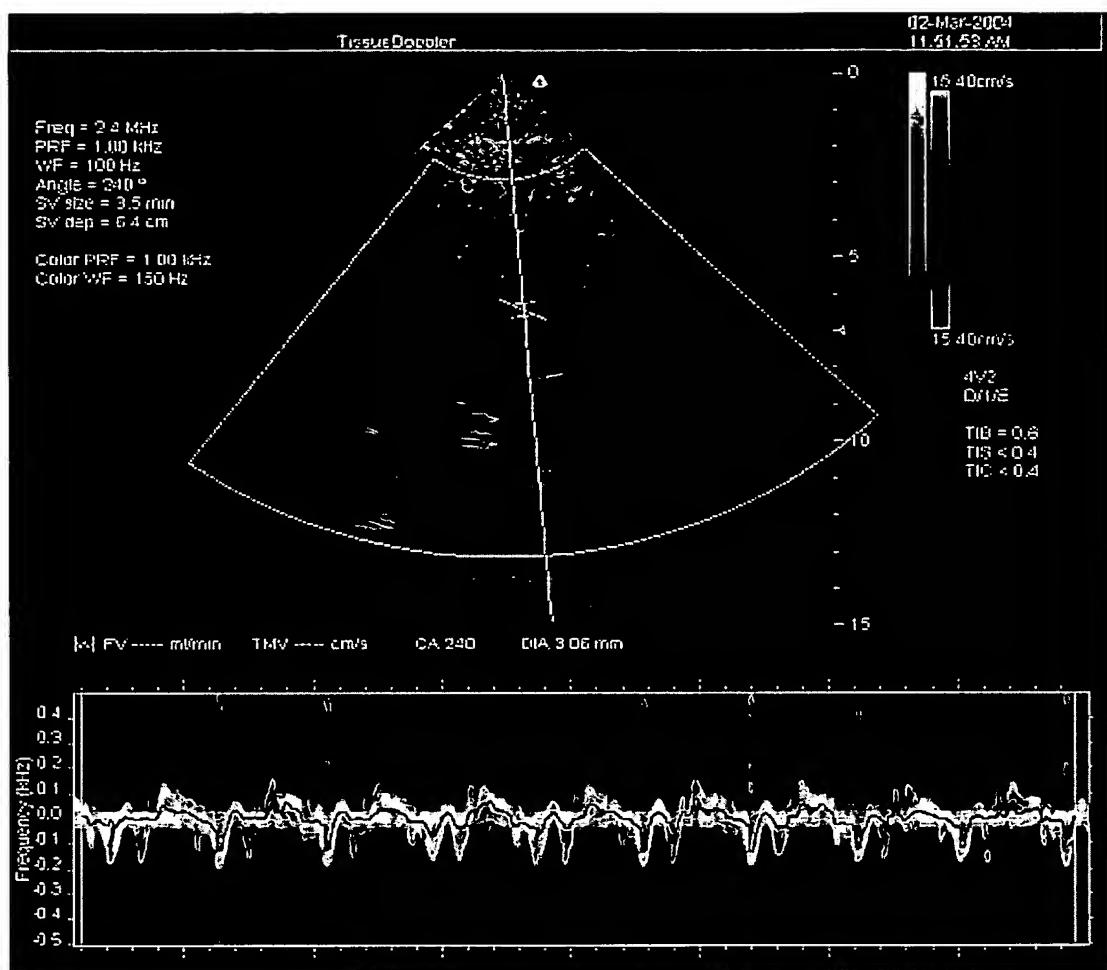


FIG. 10

13/23

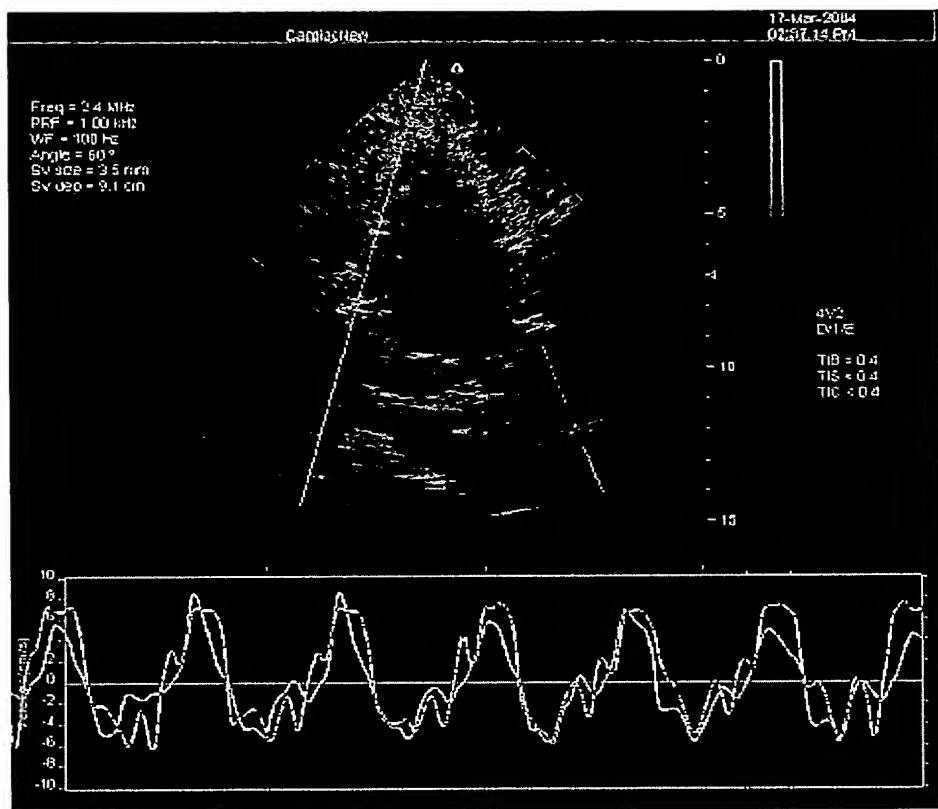


FIG. 11A

14/23

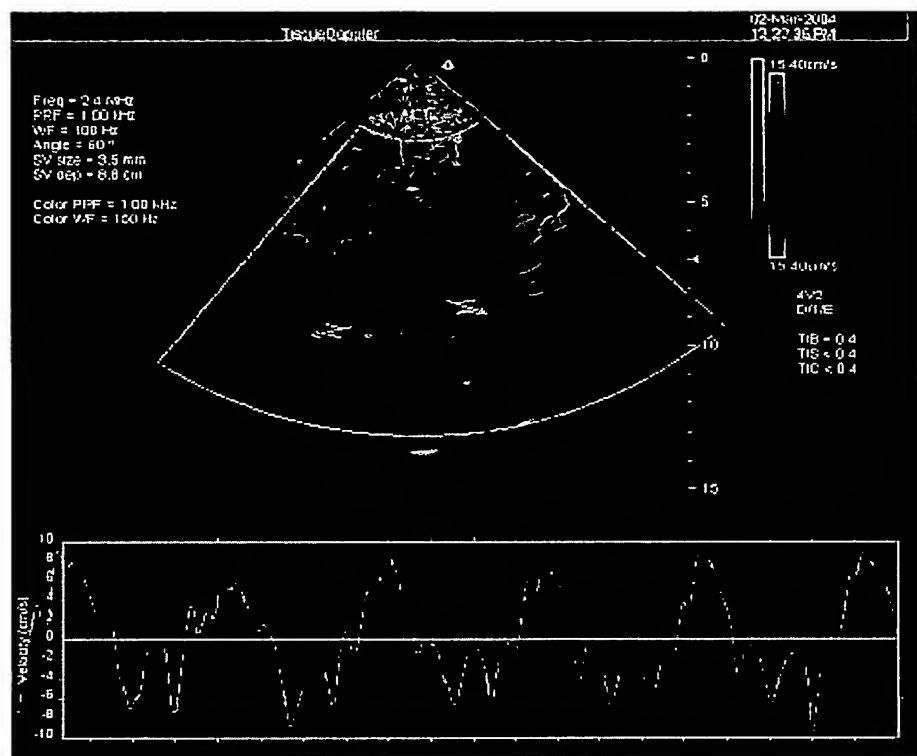


FIG. 11B

15/23

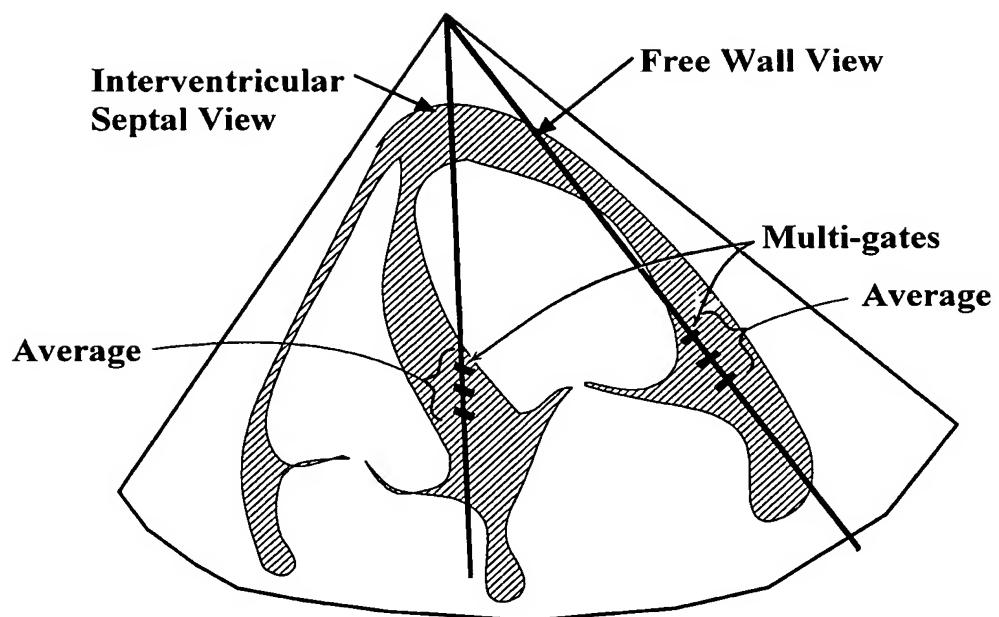


FIG. 12

16/23

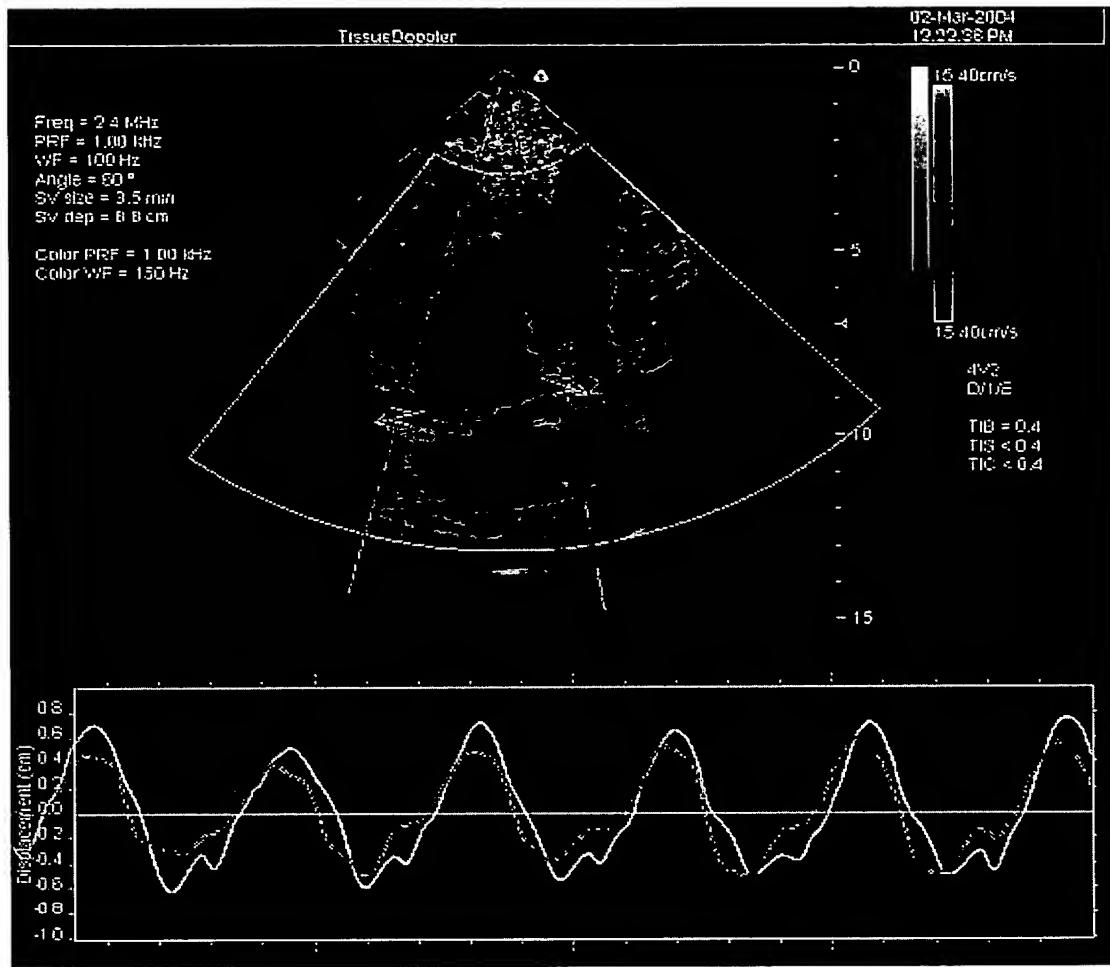


FIG. 13A

17/23

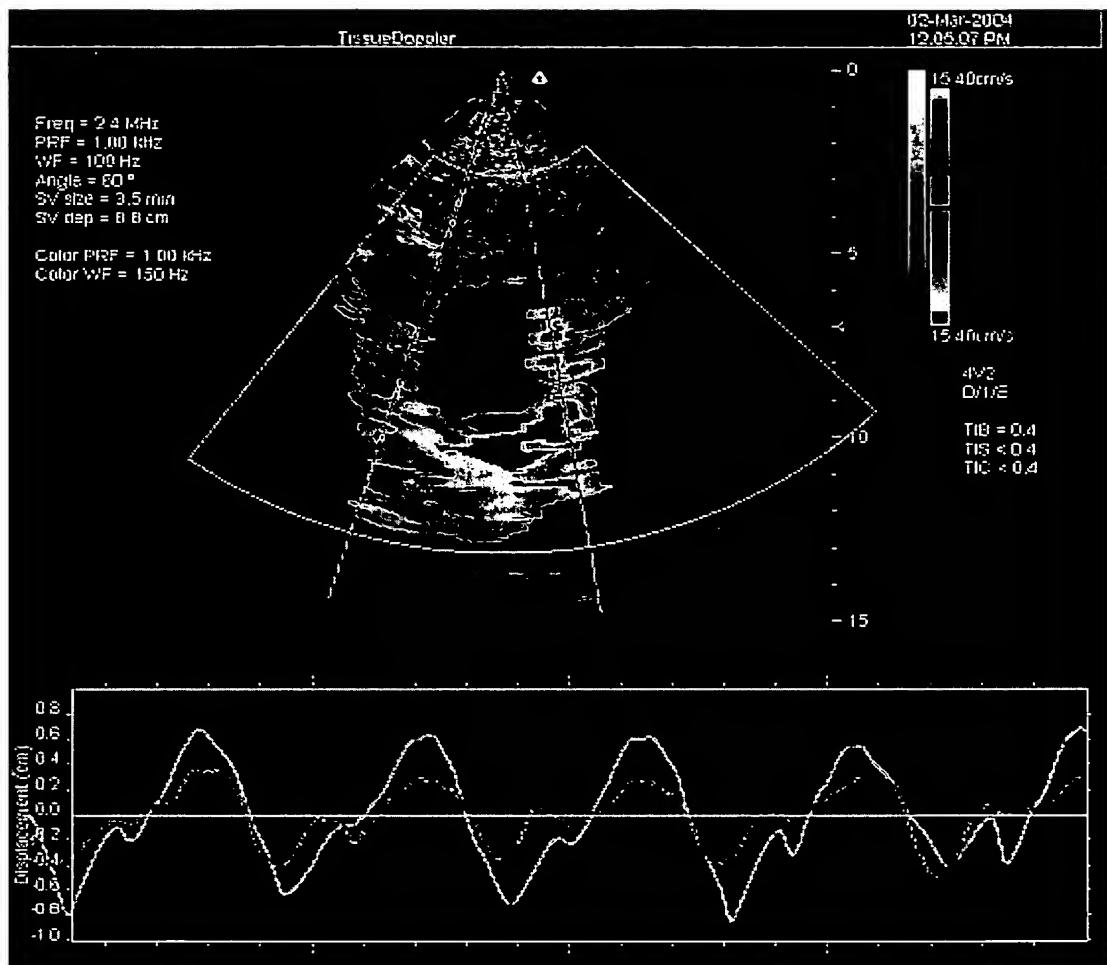


FIG. 13B

18/23

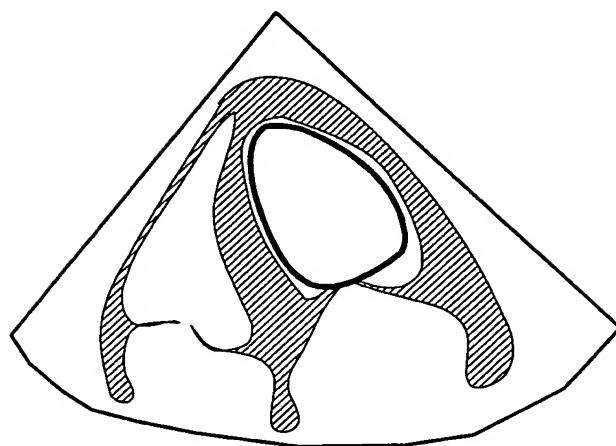


FIG. 14

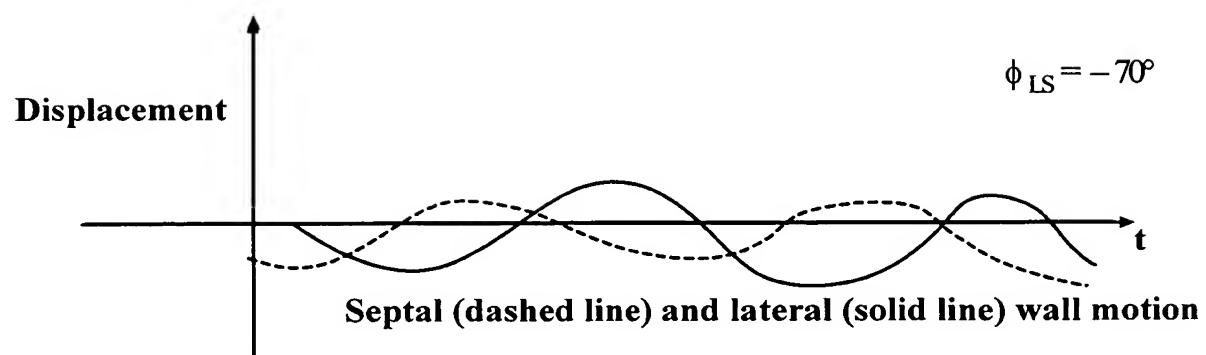


FIG. 15

19/23

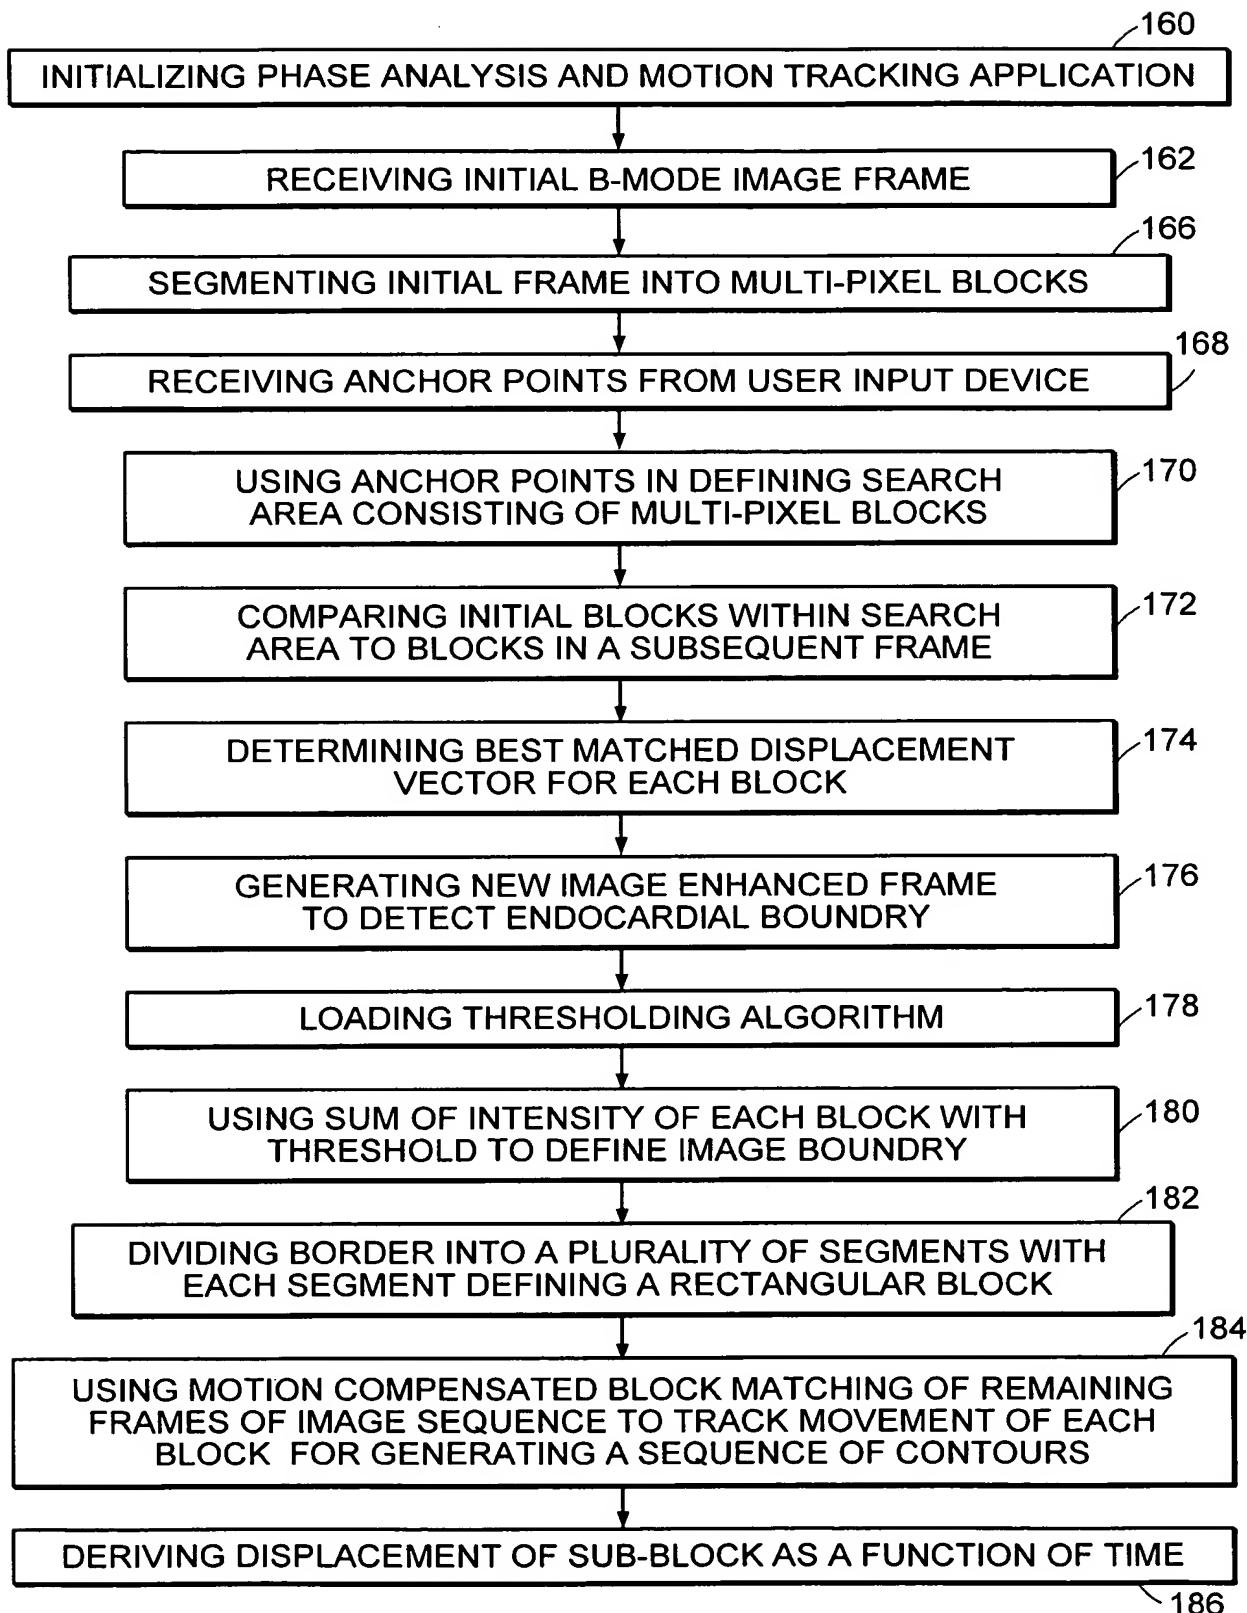


FIG. 16

20/23

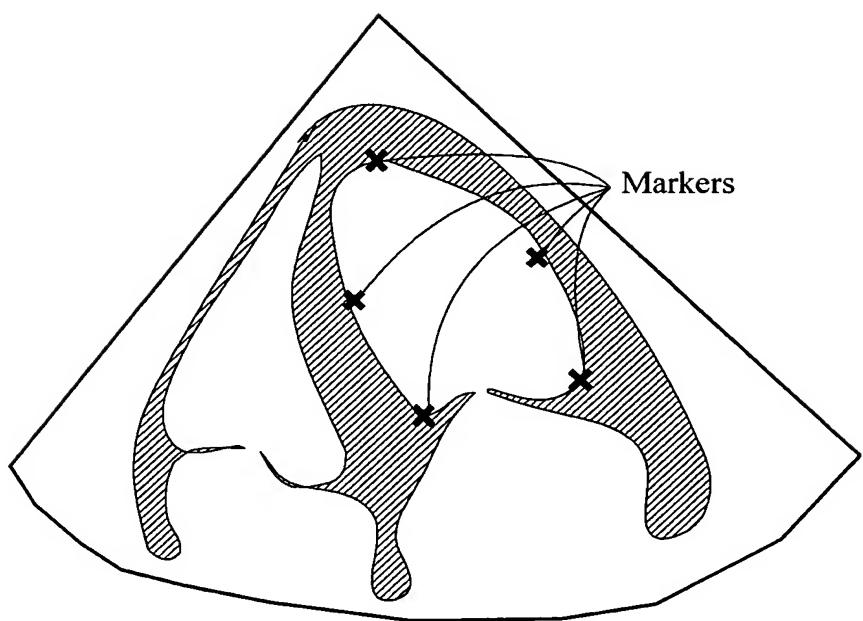


FIG. 17

21/23

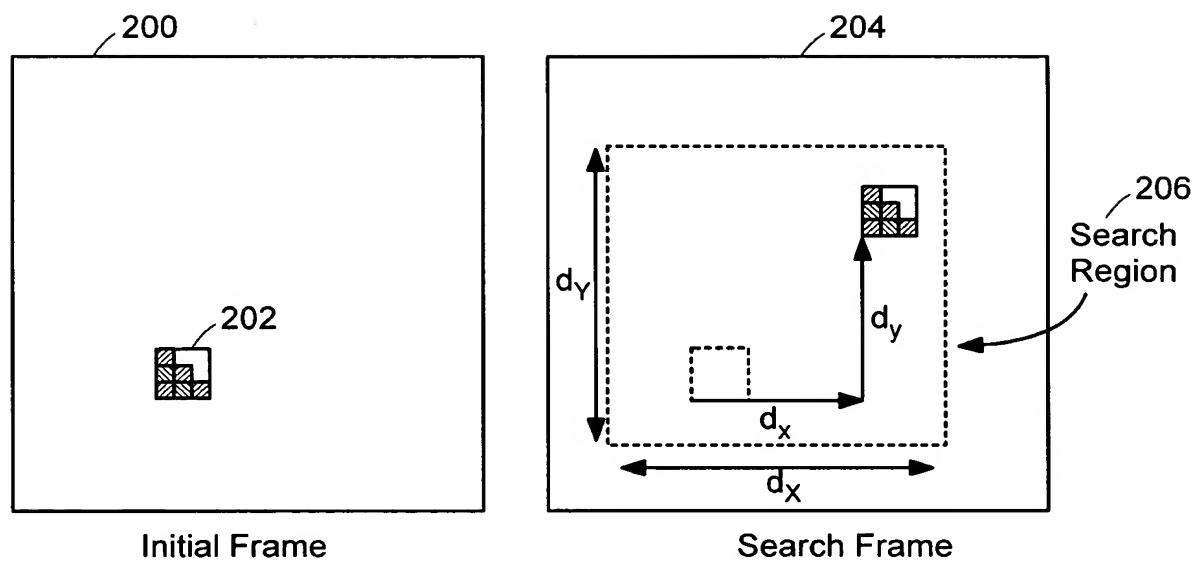


FIG. 18

22/23

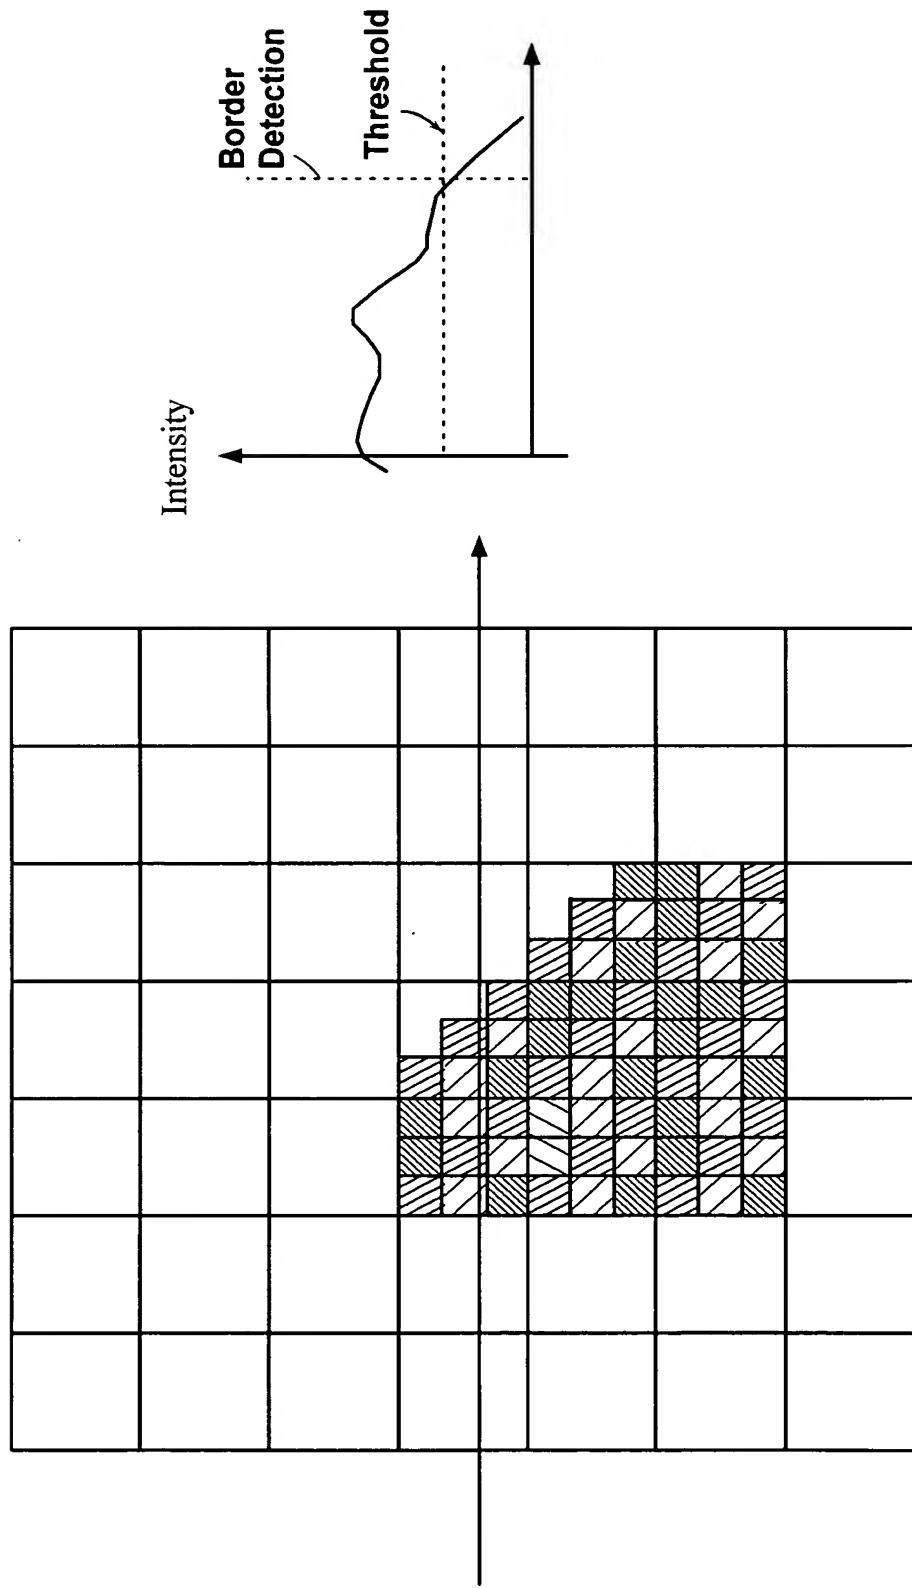


FIG. 19

23/23

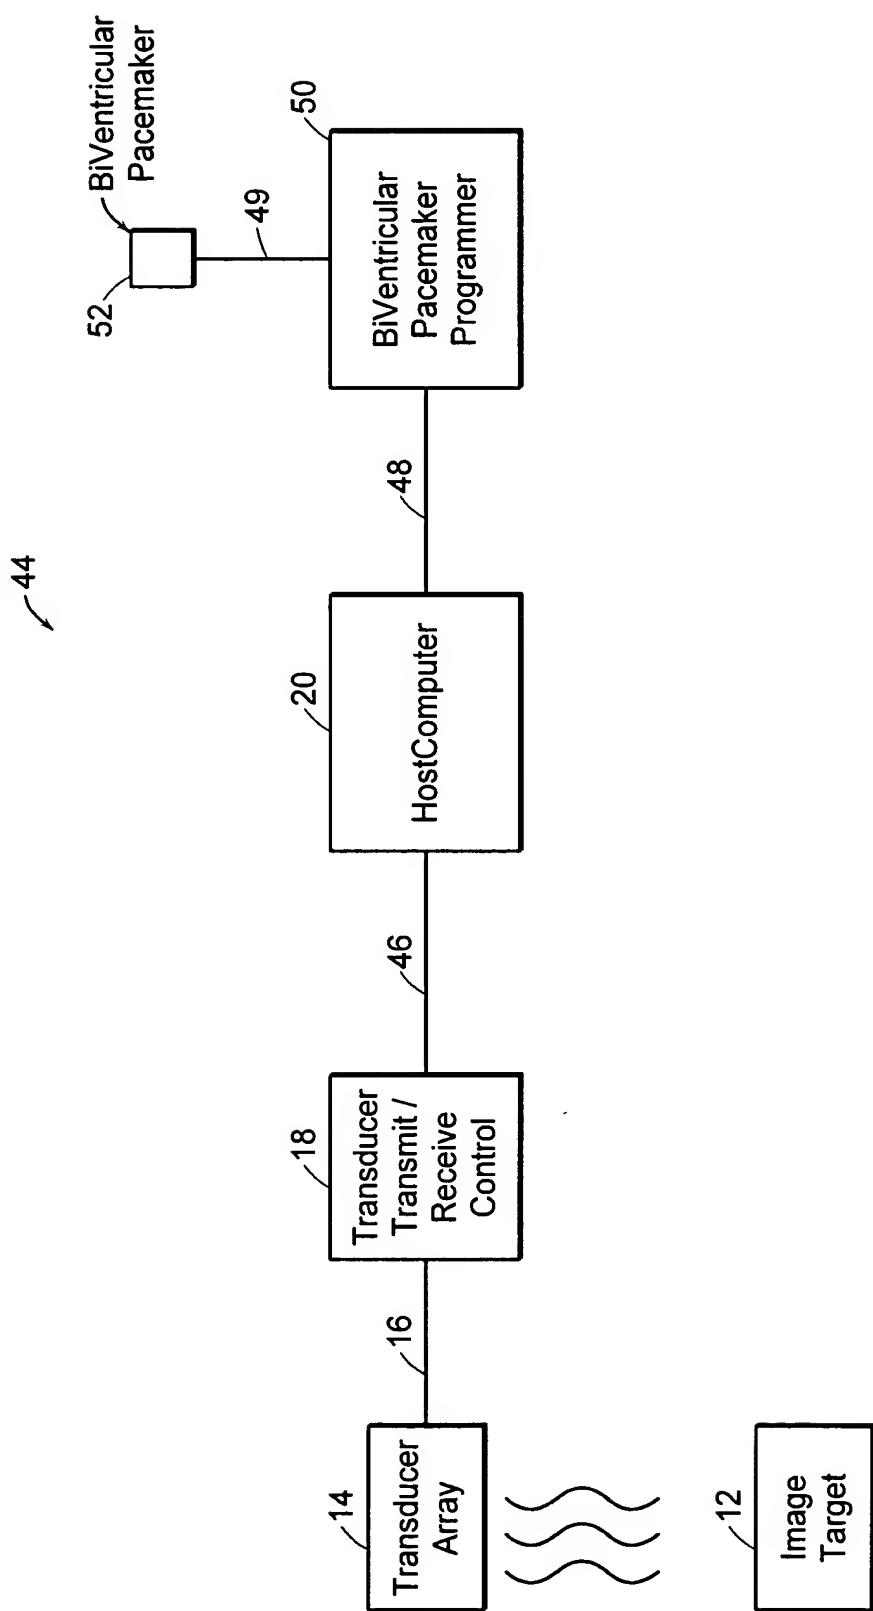


FIG. 20